

POSTER PRESENTATION

Open Access

Robust fat saturation applied to late enhancement

Martin A Janich^{1*}, Jeff A Stainsby², Glenn S Slavin³, David Stanley⁴, Christopher J Francois⁵, Scott B Reeder⁵, James F Glockner⁶, Anja C Brau⁷

From 17th Annual SCMR Scientific Sessions
New Orleans, LA, USA. 16-19 January 2014


Background

Late Gadolinium Enhancement (LGE) allows imaging of infarction and cardiomyopathies by measuring the accumulation of contrast agent within the myocardium. The shortened T_1 relaxation time compared to healthy myocardium is imaged by an inversion recovery (IR) prepared segmented fast gradient echo sequence in which pathology and fat show as bright signal. The fat signal can lead to misinterpretation and poor visualization of epicardial enhancement. In previous work fat was suppressed by using two appropriately timed fat-selective RF pulses which re-invert and invert fat signal [Foo et al., JMRI, 2007] but this technique was sensitive to off-resonance and heart rate variations. The goal of the present work is to make two improvements to fat-saturated LGE:

(1) increase robustness against B_0 and B_1 variations by using asymmetric adiabatic RF pulses, and (2) increase robustness against heart rate variations through dynamic timing of fat-selective RF pulses.

Methods

The selectivity of fat-selective pulses was improved by designing an asymmetric adiabatic inversion pulse based on HS1 and tanh/tan [Hwang et al., JMR, 1999]. This pulse had a transition width of 87 Hz which is 2 times narrower compared to a symmetric inversion pulse of the same maximum B_1 (10 μ T) and pulse duration (40 ms). M_z magnetization depends on the repetition time of the IR pulse and therefore in cardiac gated sequences depends on the patient heart rate. Heart rate variation leads to

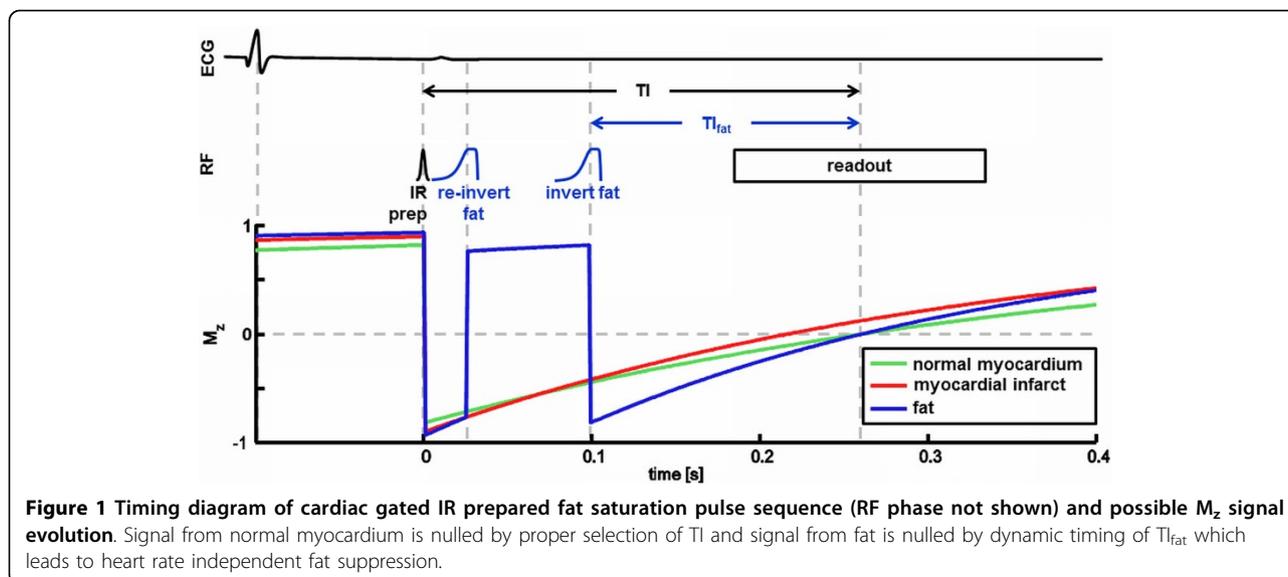

¹GE Global Research, Munich, Germany
Full list of author information is available at the end of the article

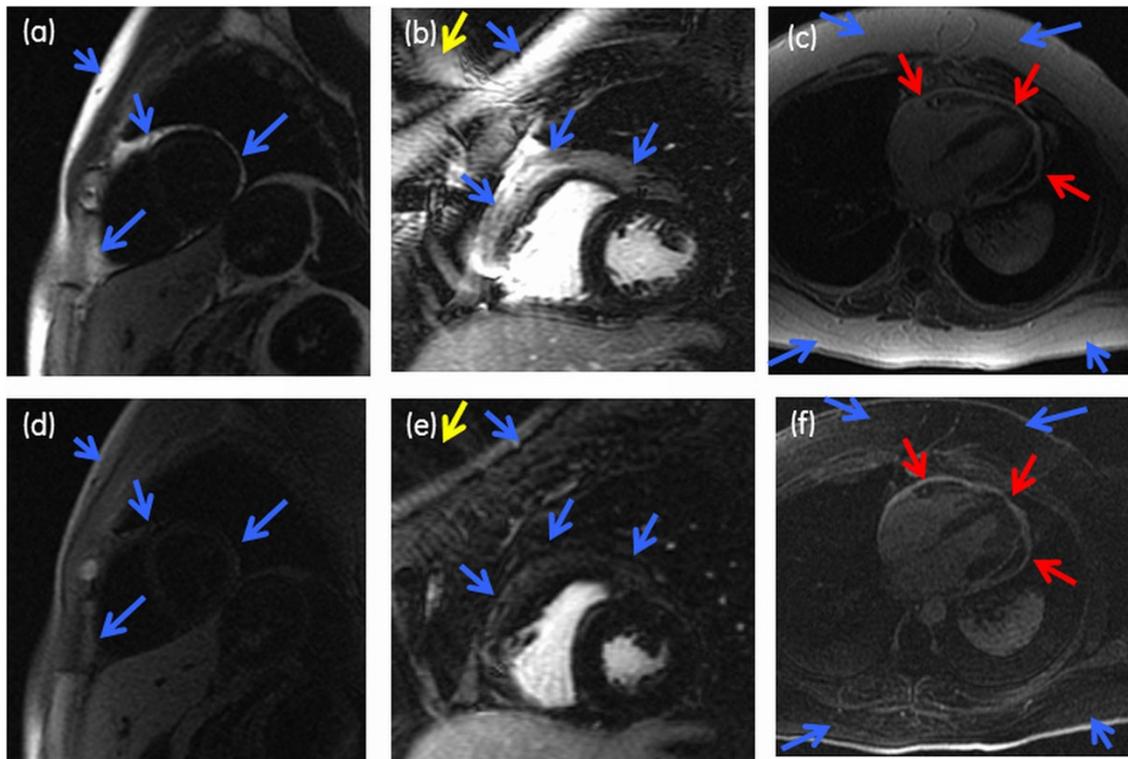


Figure 2 Short-axis IR prepared images from the heart of a (a, d) healthy volunteer (w/o contrast, 1.5T, HR \approx 60 bpm, TI 280 ms), (b, e) patient (w/contrast, 3.0T, HR \approx 60 bpm, TI 290 ms), and (e, f) patient with pericardial enhancement (w/contrast, 1.5T, HR \approx 80 bpm, TI 260 ms). The upper row images (a-c) were acquired with IR preparation only and the lower row images (d-f) were acquired with IR preparation and fat saturation. The new technique led to suppression of normal myocardium and fat signal (blue arrows) which avoided image wrapping of subcutaneous fat (e, yellow arrows) and better visualization of pericardial enhancement (f, red arrows).

a shifting of the inversion time (TI_{fat}) at which the fat signal is nulled. Therefore a heart rate independent nulling of fat signal was developed by measuring the length of each R-R interval during the examination and time-shifting the fat-selective inversion pulse accordingly (Figure 1). The method was tested in volunteers without contrast and patients with contrast on 1.5T (MR450w) and 3.0T (MR750) MR systems (GE Healthcare).

Results

The $T_{1,fat}$ value which influences the heart rate-dependent TI_{fat} was calibrated in healthy volunteers at field strengths 1.5T (220 ms) and 3.0T (300 ms). With appropriate TI selection the technique led to nulling of signal from healthy myocardium and from fat. The cases without contrast injection had poor blood-myocardium contrast due to the lack of Gd (Figure 2(a)) but fat was successfully suppressed.

Conclusions

Benefits of fat-saturated LGE imaging include avoiding image wrapping of subcutaneous fat and therefore reduced possible misdiagnosis (Figure 2(b)), and in patients with

pericardial enhancement the ability to rule out epicardial fat and better visualization of pathology (Figure 2(c)). The selectivity improvement of fat-selective pulses was particularly important at 1.5T where the chemical shift difference between fat and water is only 220 Hz. The technique presented here was proven to be robust in more than 20 cases.

Authors' details

¹GE Global Research, Munich, Germany. ²GE Healthcare, Toronto, Ontario, Canada. ³GE Healthcare, Bethesda, Maryland, USA. ⁴GE Healthcare, Rochester, Minnesota, USA. ⁵Radiology, University of Wisconsin, Madison, Wisconsin, USA. ⁶Mayo Clinic, Rochester, Minnesota, USA. ⁷GE Healthcare, Munich, Germany.

Published: 16 January 2014

doi:10.1186/1532-429X-16-S1-P196

Cite this article as: Janich et al.: Robust fat saturation applied to late enhancement. *Journal of Cardiovascular Magnetic Resonance* 2014 16(Suppl 1):P196.