

WORKSHOP PRESENTATION

Open Access

Synchronized cardiac and respiratory sparsity for rapid free-breathing cardiac cine MRI


Li Feng^{1*}, Leon Axel¹, Jian Xu², Daniel K Sodickson¹, Ricardo Otazo¹

From 17th Annual SCMR Scientific Sessions
New Orleans, LA, USA. 16-19 January 2014

Background

For patients with impaired breath-hold capacity or arrhythmias, free breathing real-time cine MRI is preferred at the expense of compromised spatiotemporal

resolution. Compressed sensing (CS) has been used to achieve higher spatiotemporal resolutions in real-time cine MRI, but the superposition of respiratory and cardiac motion limits temporal sparsity. In this work, we

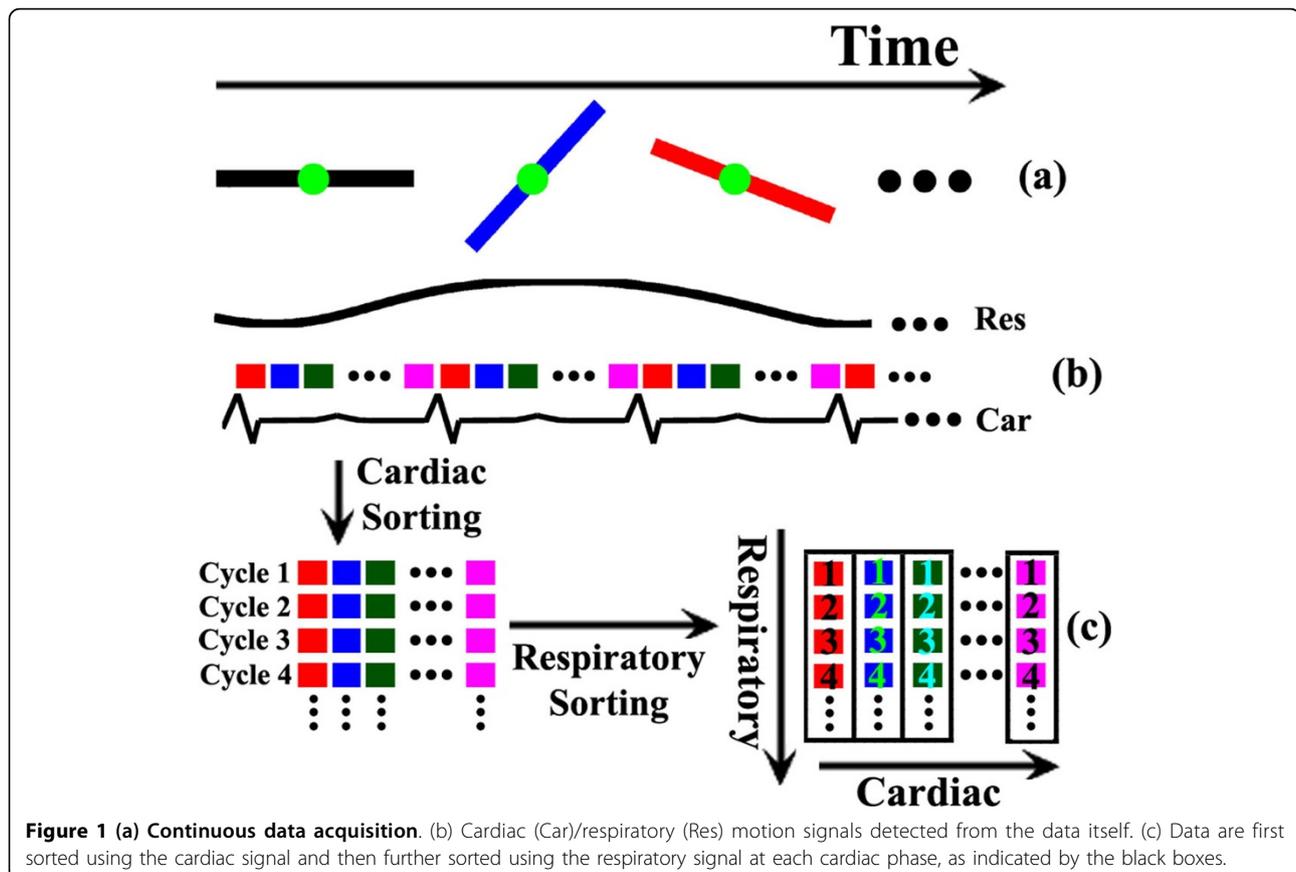

¹Bernard and Irene Schwartz Center for Biomedical Imaging, New York University School of Medicine, New York, New York, USA
Full list of author information is available at the end of the article

propose a novel approach that sorts out cardiac and respiratory motion into separated but synchronized dimensions and performs a joint multicoil CS reconstruction with different sparsity constraints on cardiac and respiratory dimensions. Golden-angle radial sampling was employed for flexible data sorting. In arrhythmias cases, data are also sorted according to cardiac cycles with different length to reconstruct both “normal” and “ectopic” cycles.

Methods

Cardiac imaging was performed on one volunteer (male age = 27) and one patient (female age = 49) with Mobitz I arrhythmia during free breathing without external gating on a 1.5T MRI scanner (Avanto, Siemens). Data were continuously acquired for 15 s in a short axis plane using a 2D golden-angle radial b-SSFP sequence. Imaging parameters were: spatial resolution = $2 \times 2 \text{ mm}^2$, TR/TE = 2.8/1.4 ms, FA = 70° and slice thickness = 8 mm. Temporal

evolution of the central k-space positions (green dots, Figure 1a) was used to estimate cardiac contraction and respiration from coil-elements close to the heart and diaphragm respectively (Figure 1b). Raw data were then sorted into an expanded dataset of images containing two dynamic dimensions, one for cardiac and the other for respiratory motion. As shown in Figure 1b, each colored rectangular block represents an individual cardiac phase from a short “snapshot” period (e.g. 13 adjacent spokes). Data were sorted first into a higher dimensional matrix using the cardiac motion signal (Figure 1c left) followed by a second sorting along the respiratory dimension from expiration to inspiration using the respiratory motion signal, performed within each black box shown in Figure 1c (right). For the arrhythmia patient, data from both “normal” and “ectopic” cycles were sorted separately according to the length of cardiac cycles so that reconstruction could be performed separately to produce both “normal” and “ectopic” cycles. CS reconstruction was performed with

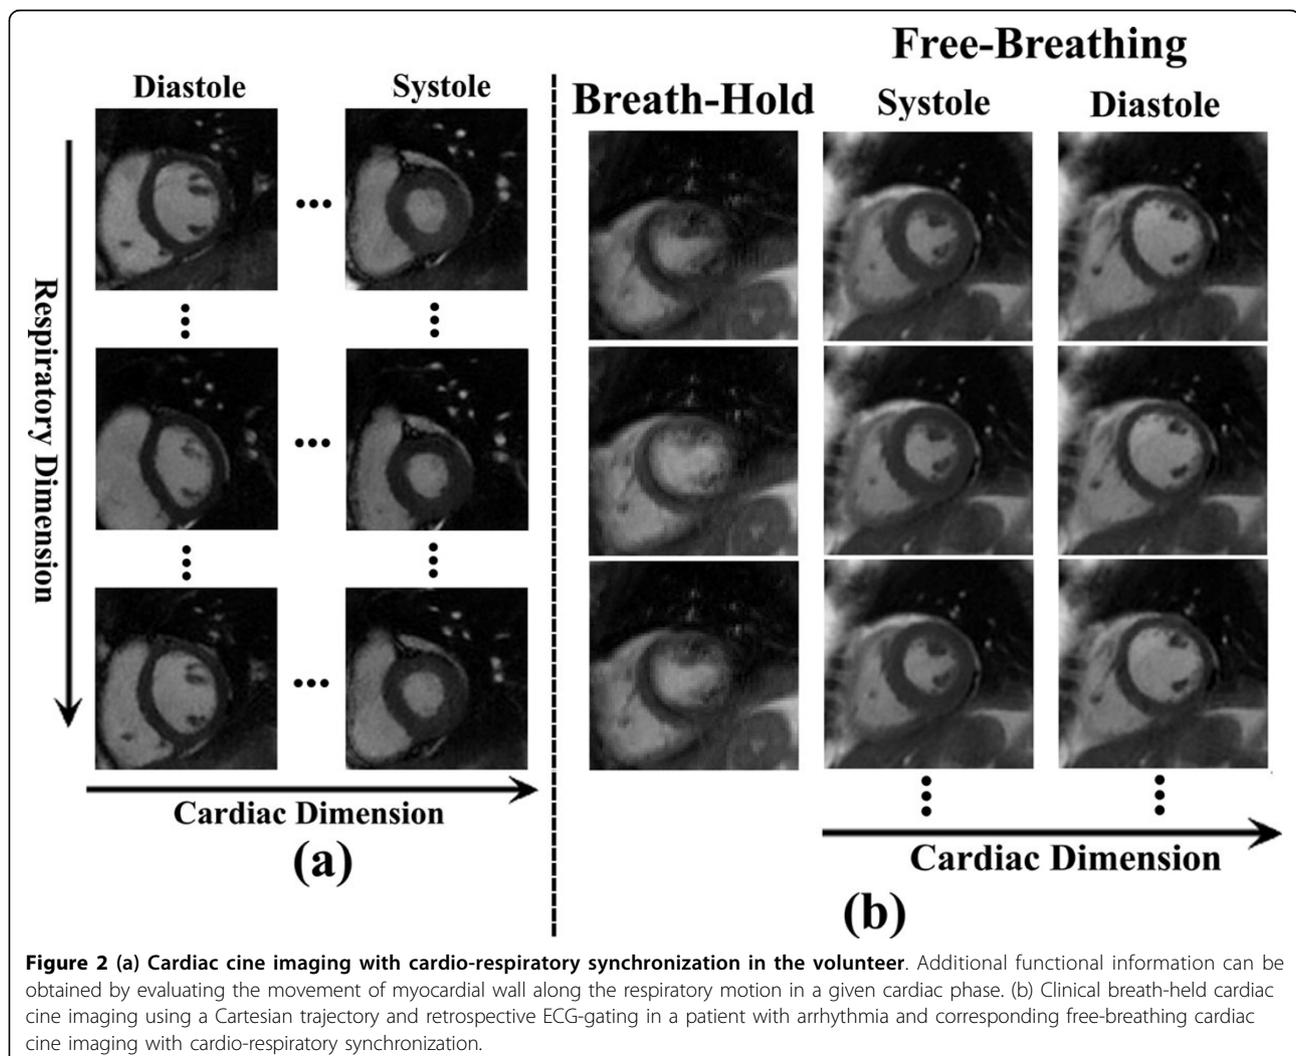


Figure 2 (a) Cardiac cine imaging with cardio-respiratory synchronization in the volunteer. Additional functional information can be obtained by evaluating the movement of myocardial wall along the respiratory motion in a given cardiac phase. (b) Clinical breath-held cardiac cine imaging using a Cartesian trajectory and retrospective ECG-gating in a patient with arrhythmia and corresponding free-breathing cardiac cine imaging with cardio-respiratory synchronization.

two total variation constraints along cardiac and respiratory dimensions. The results were also compared to Cartesian breath-hold approach using retrospective ECG-gating.

Results

Figure 2a shows the different cardiac phases and respiratory states on the volunteer. Figure 2b compares the clinical breath-hold approach with the proposed method on the patient. Superior image quality is achieved even in the presence of arrhythmia.

Conclusions

Separating cardiac and respiratory motion improved the sparsity of representation and thus the acceleration capability for CS. Additional functional information can be obtained by evaluating the movement of myocardial wall along the respiratory motion in a given cardiac phase.

Authors' details

¹Bernard and Irene Schwartz Center for Biomedical Imaging, New York University School of Medicine, New York, New York, USA. ²Siemens Medical Solutions, New York, New York, USA.

Published: 16 January 2014

doi:10.1186/1532-429X-16-S1-W26

Cite this article as: Feng *et al.*: Synchronized cardiac and respiratory sparsity for rapid free-breathing cardiac cine MRI. *Journal of Cardiovascular Magnetic Resonance* 2014 **16**(Suppl 1):W26.

**Submit your next manuscript to BioMed Central
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

